

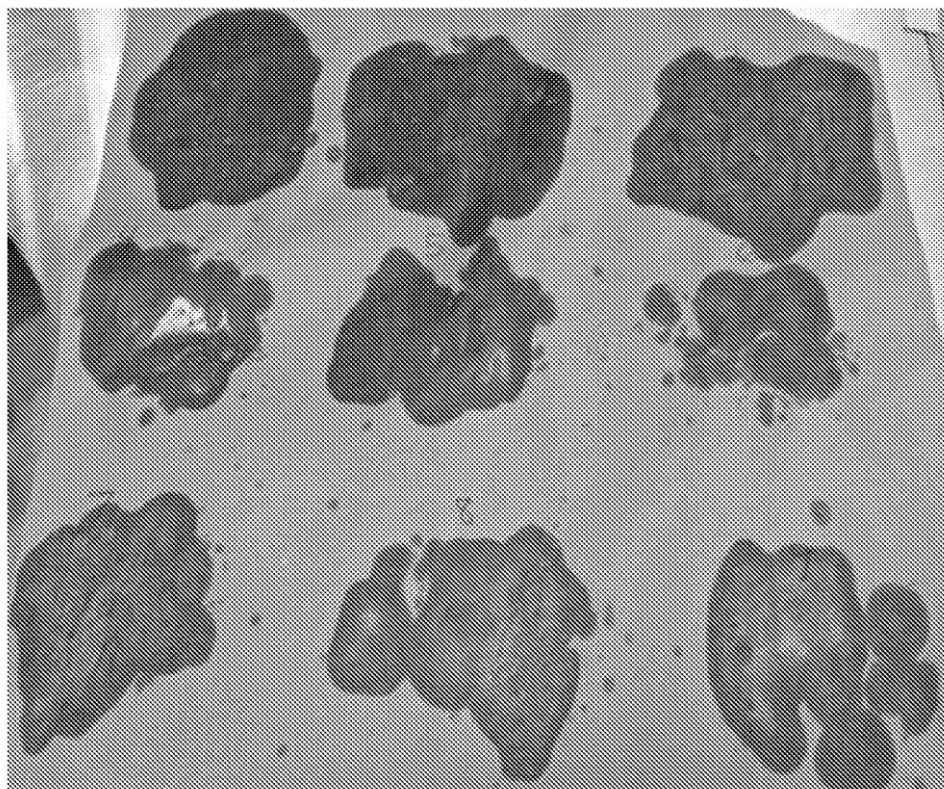


FIG. 1

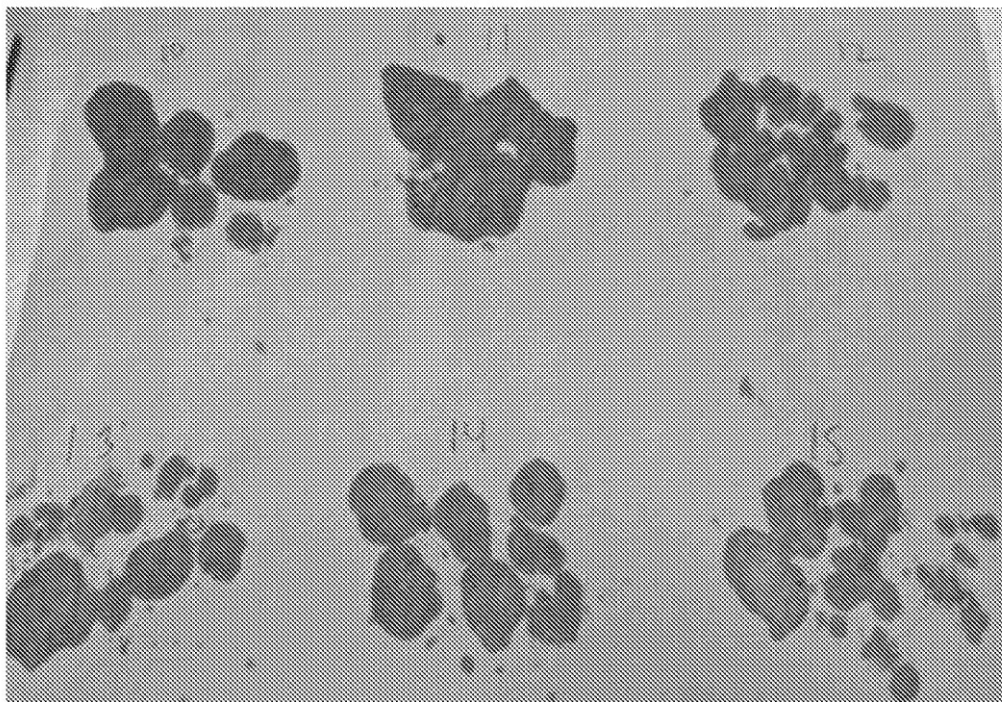


FIG. 2

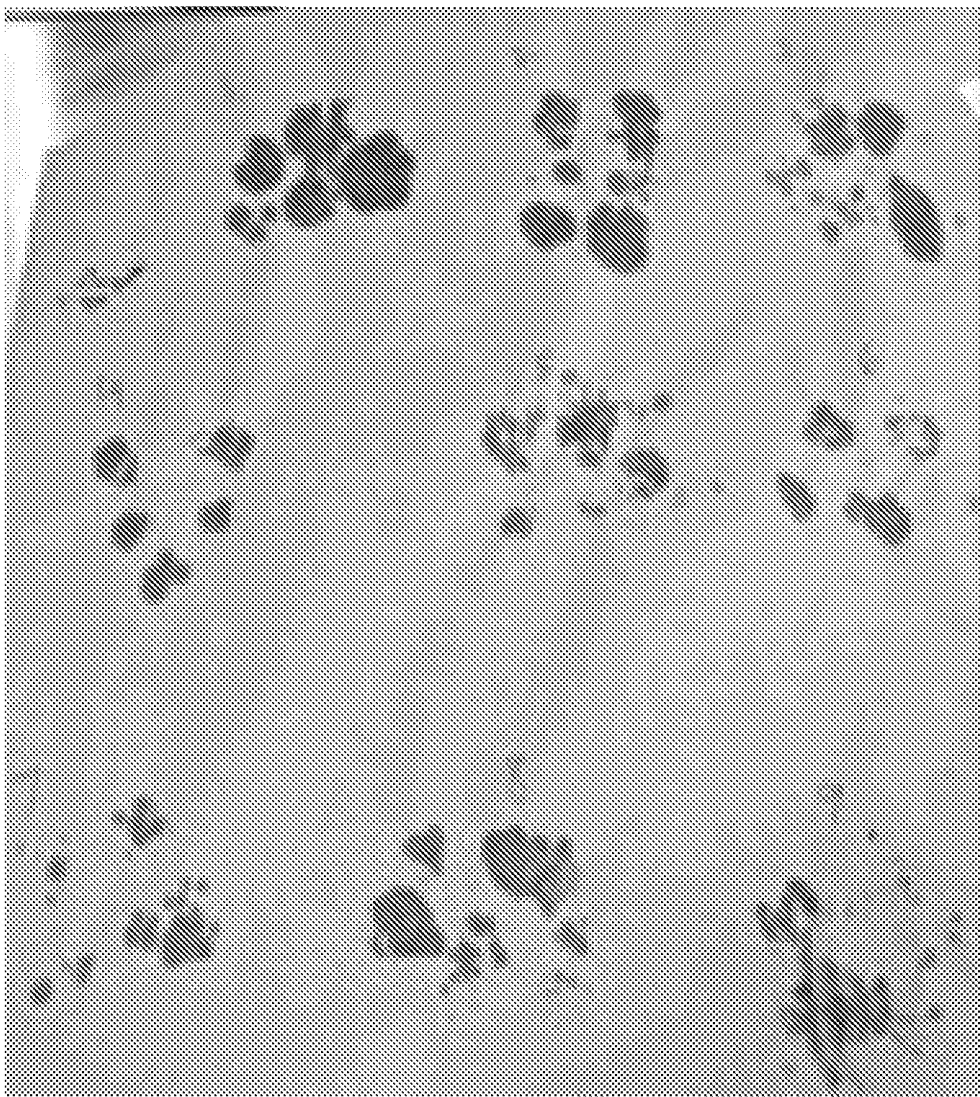


FIG. 3

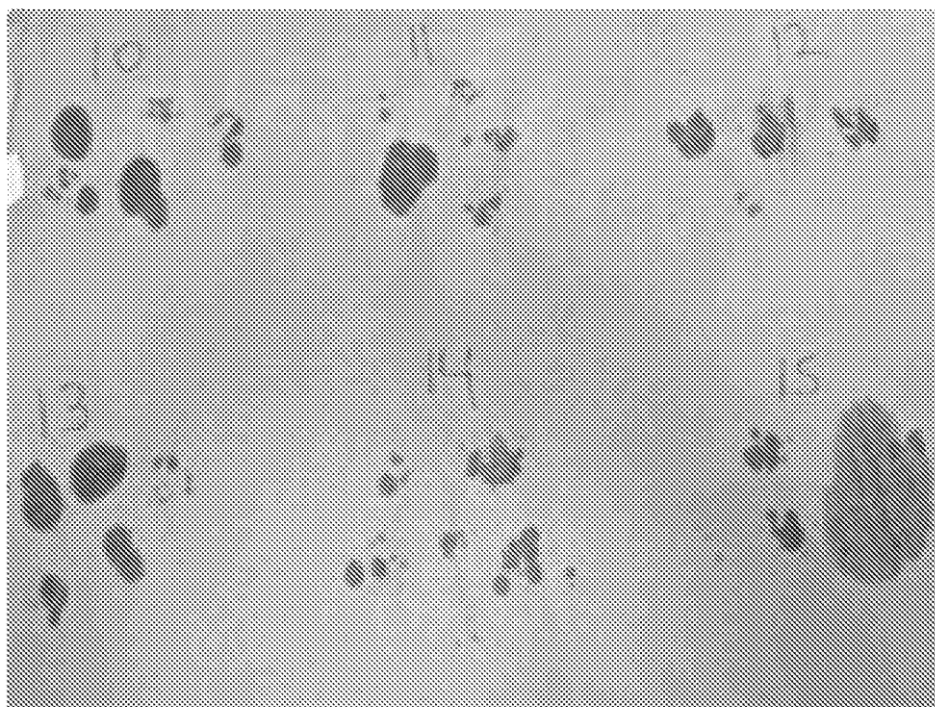


FIG. 4



FIG. 5

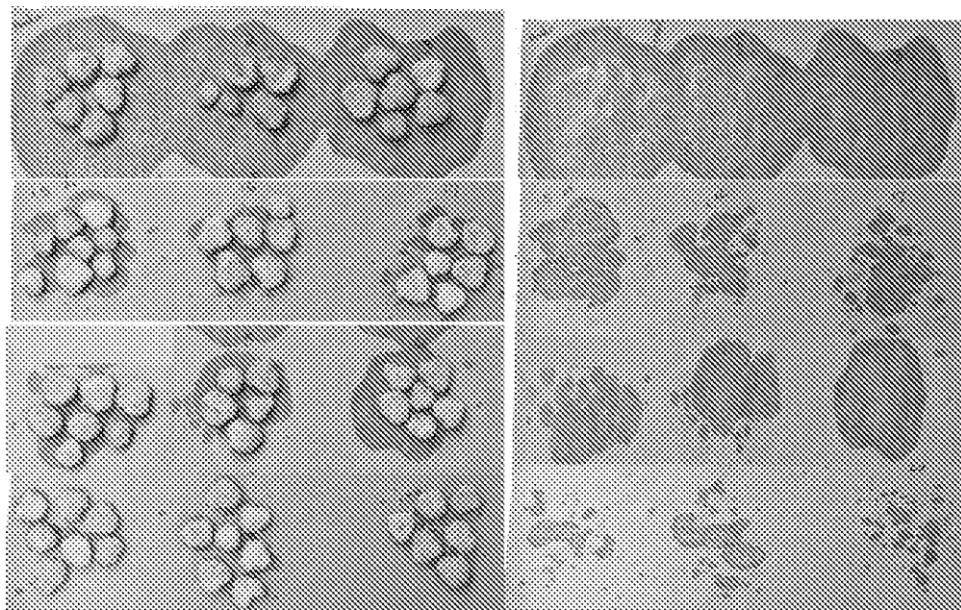


FIG. 6.

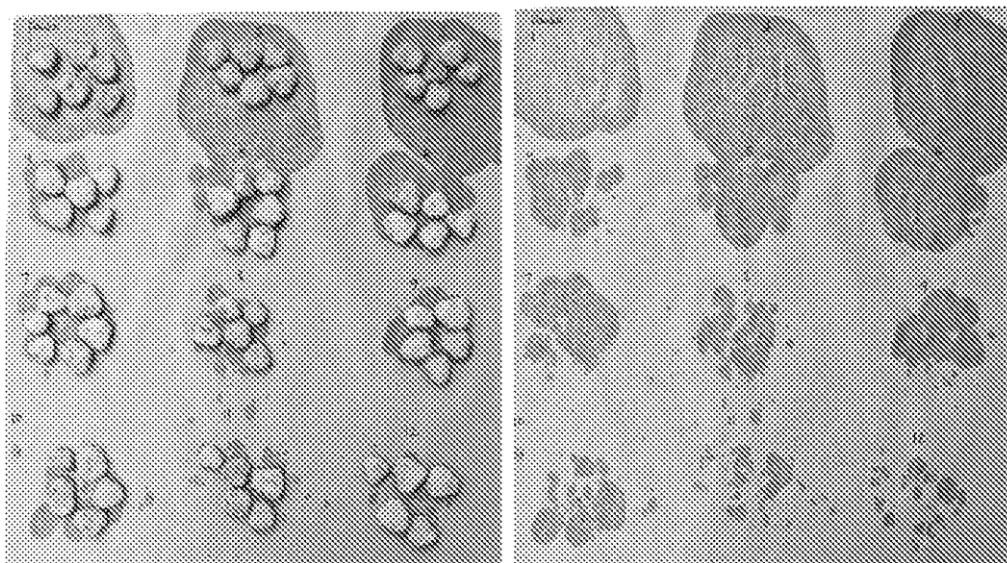


FIG. 7

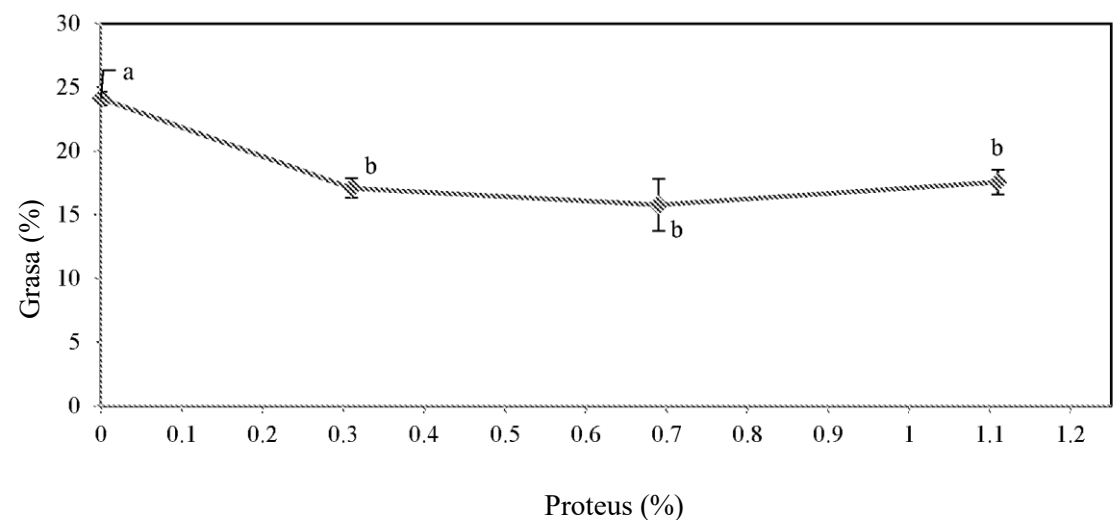


FIG. 8

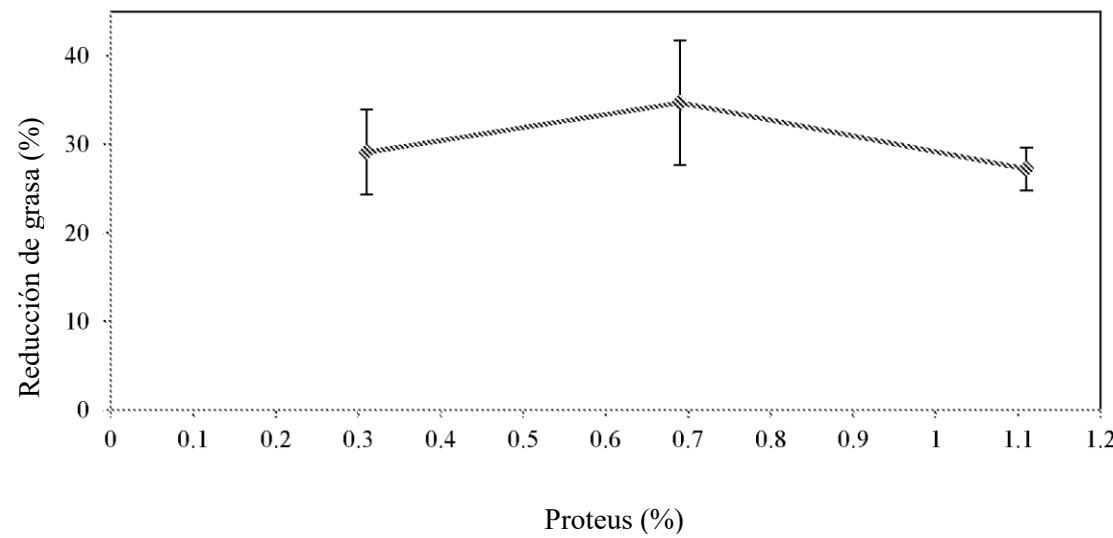


FIG. 9

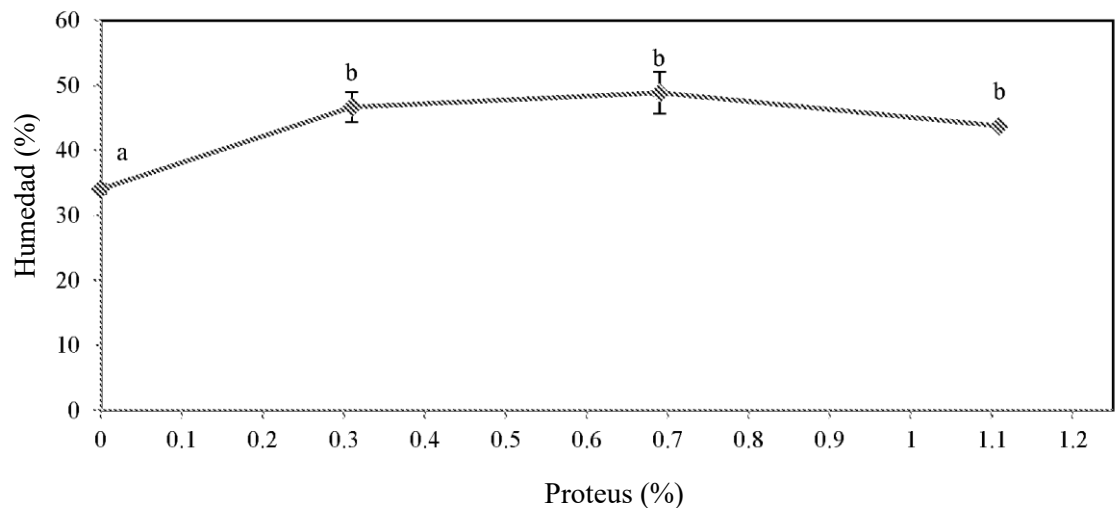


FIG. 10

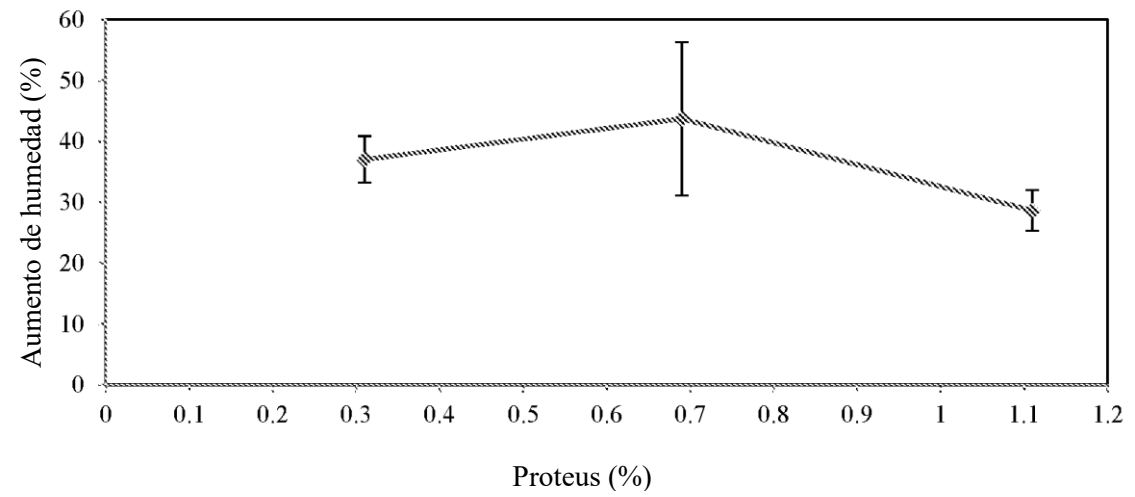


FIG. 11

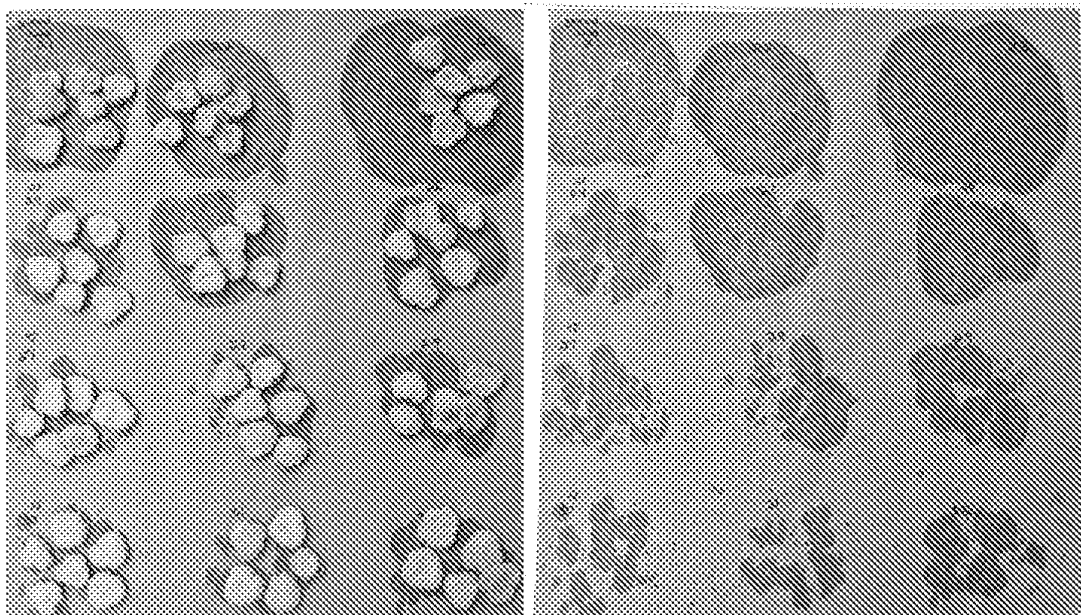


FIG. 12

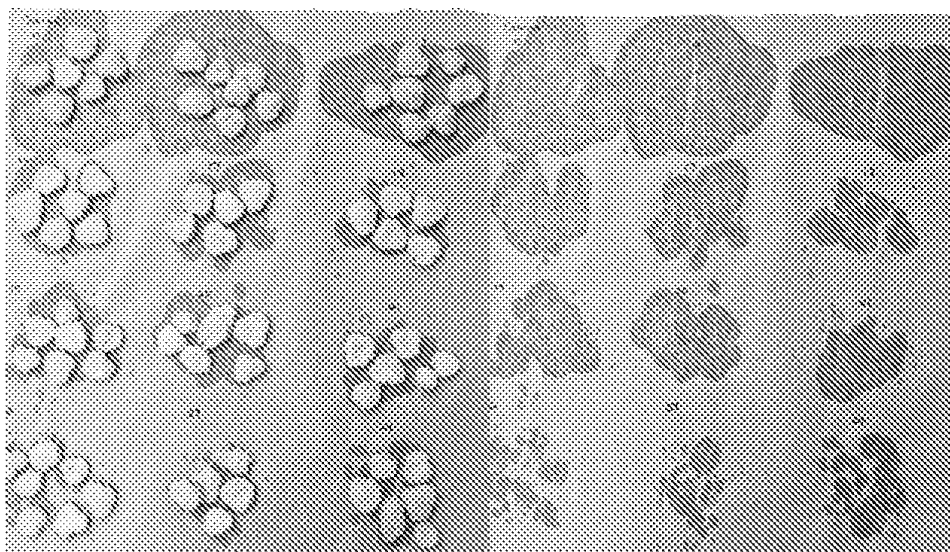


FIG. 13

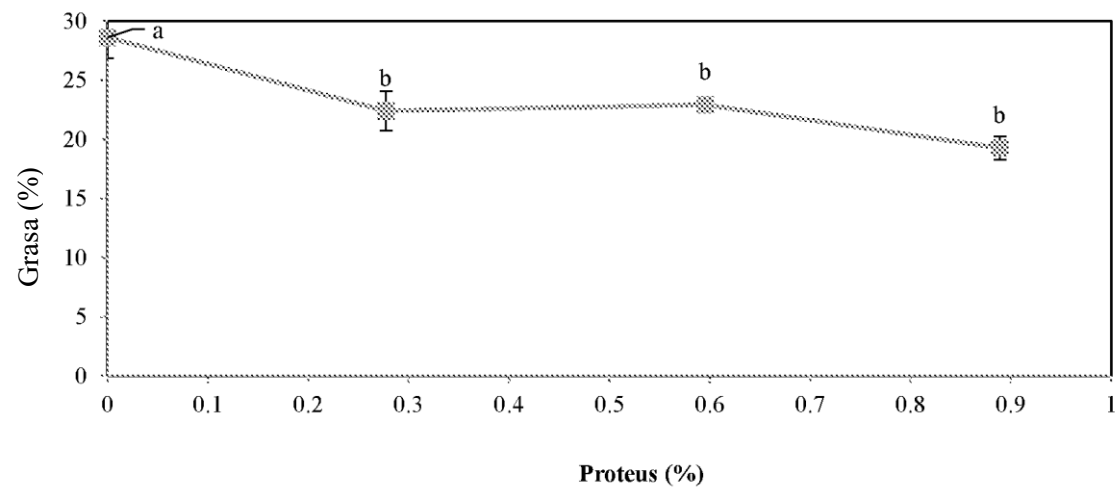


FIG. 14

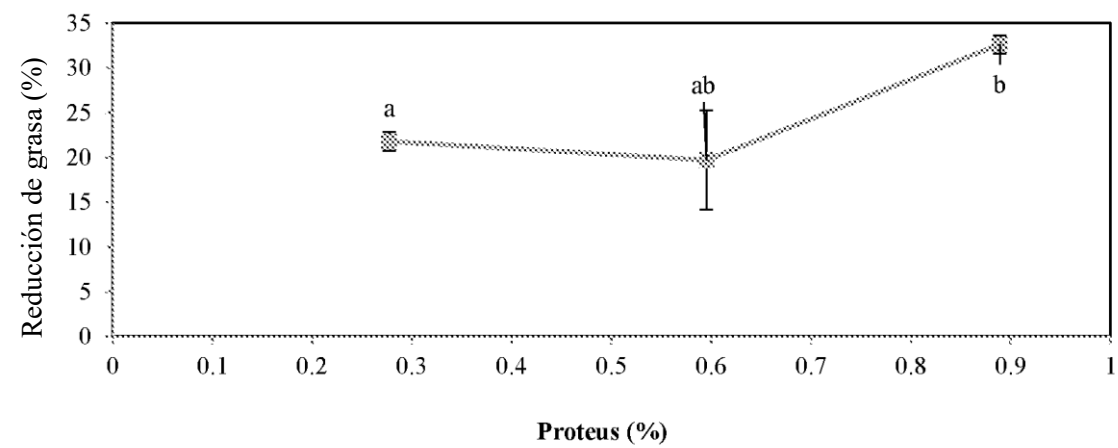


FIG. 15

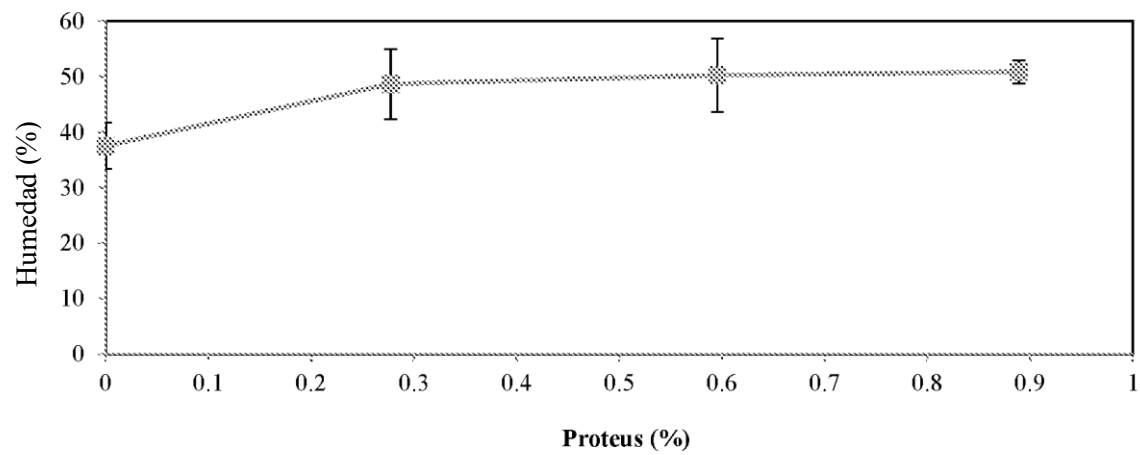


FIG. 16

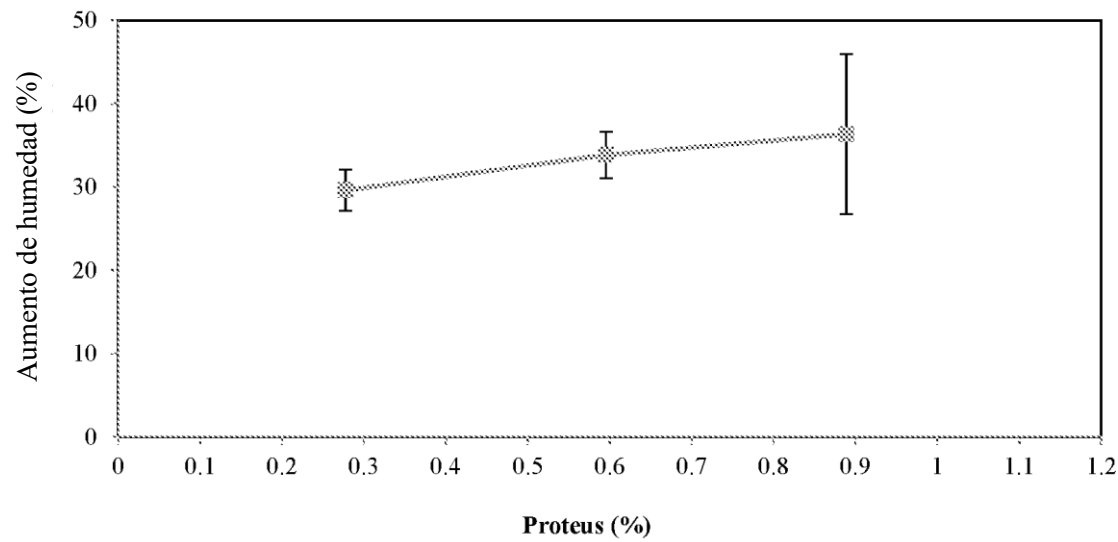


FIG. 17

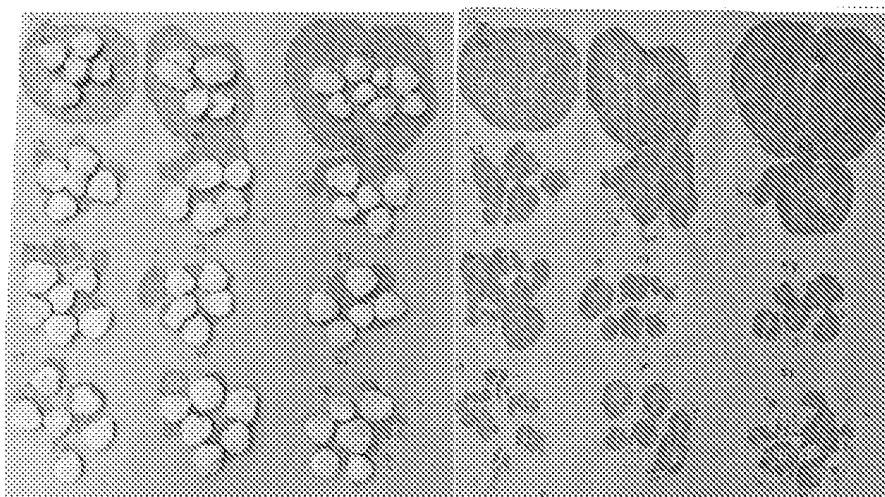


FIG. 18

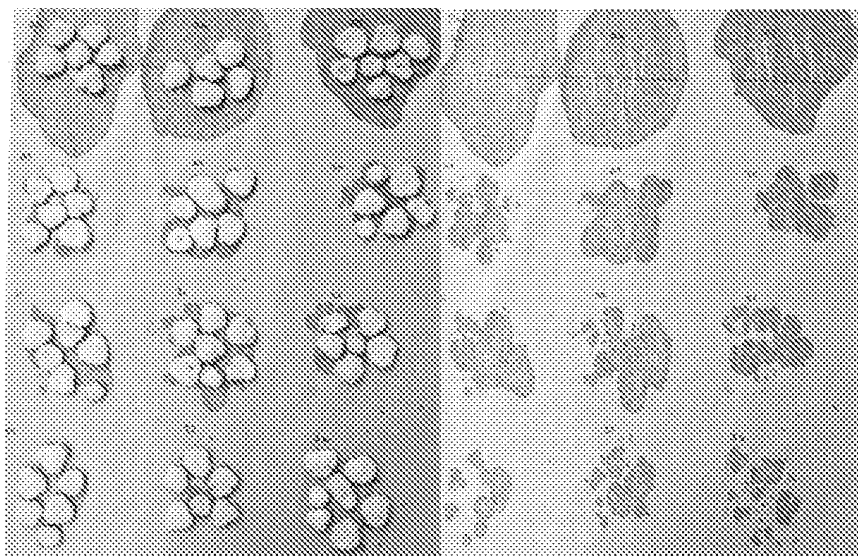


FIG. 19

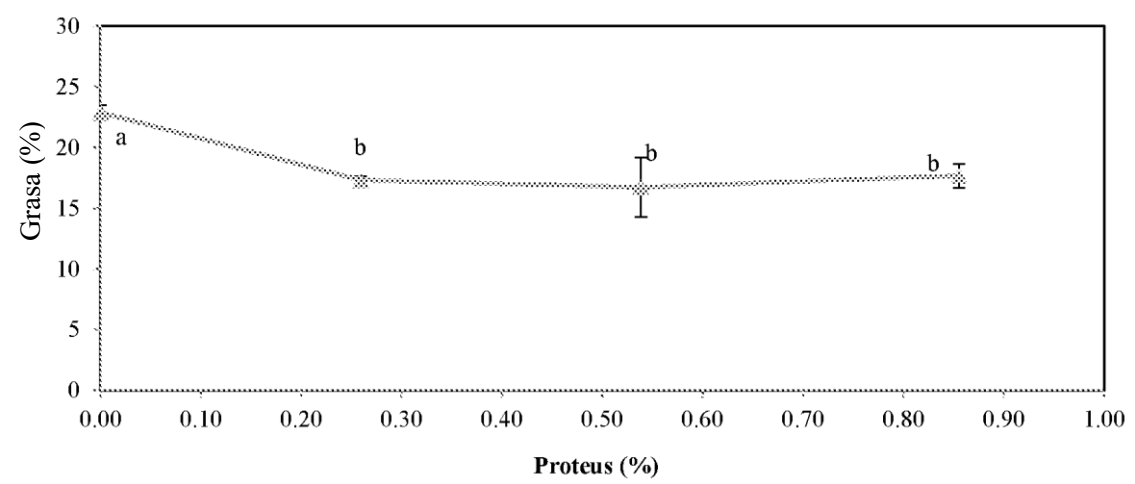


FIG. 20

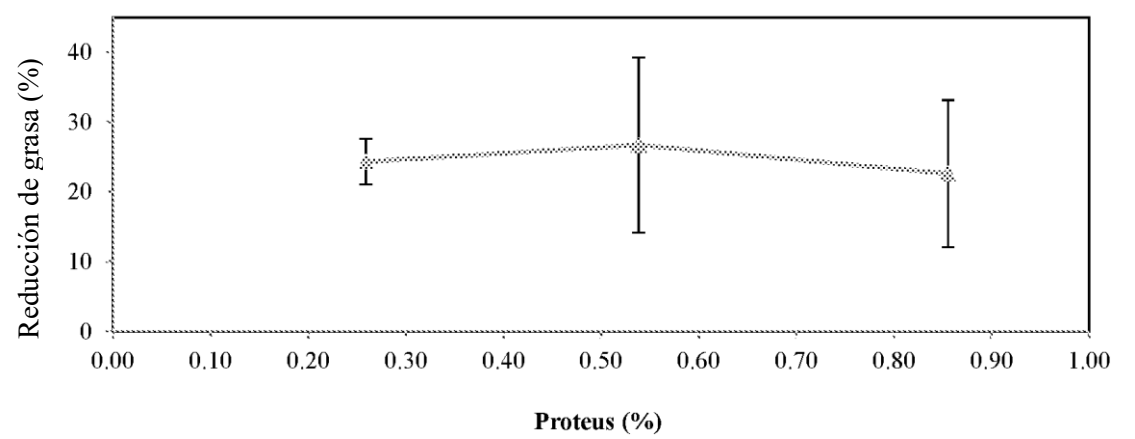


FIG. 21

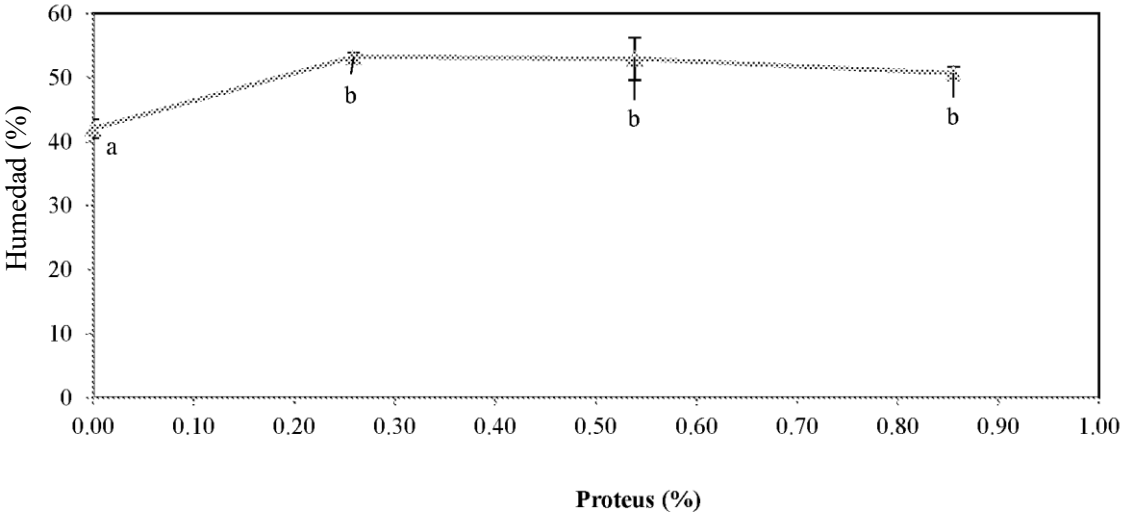


FIG. 22

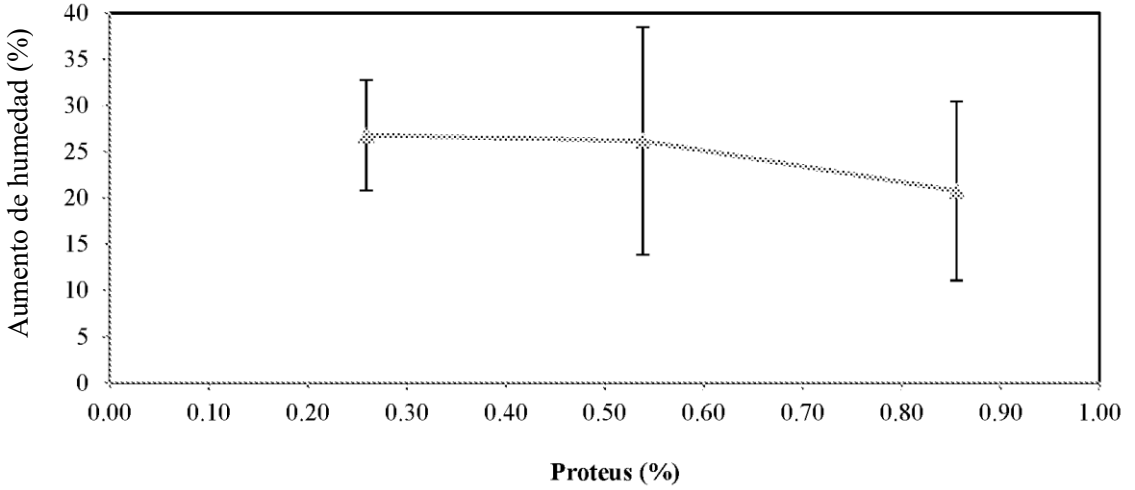


FIG. 23

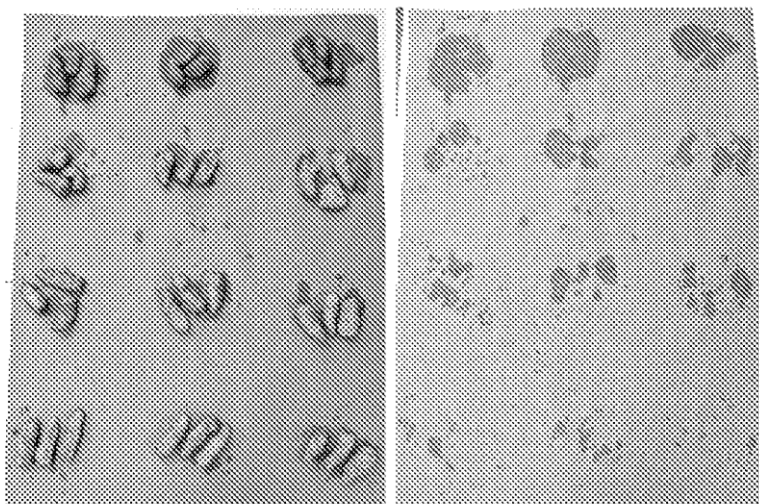


FIG. 24

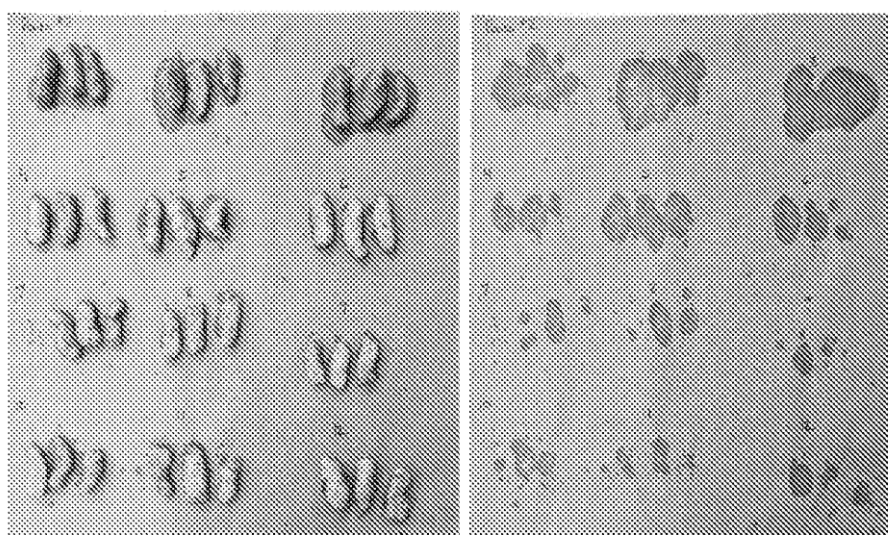


FIG. 25

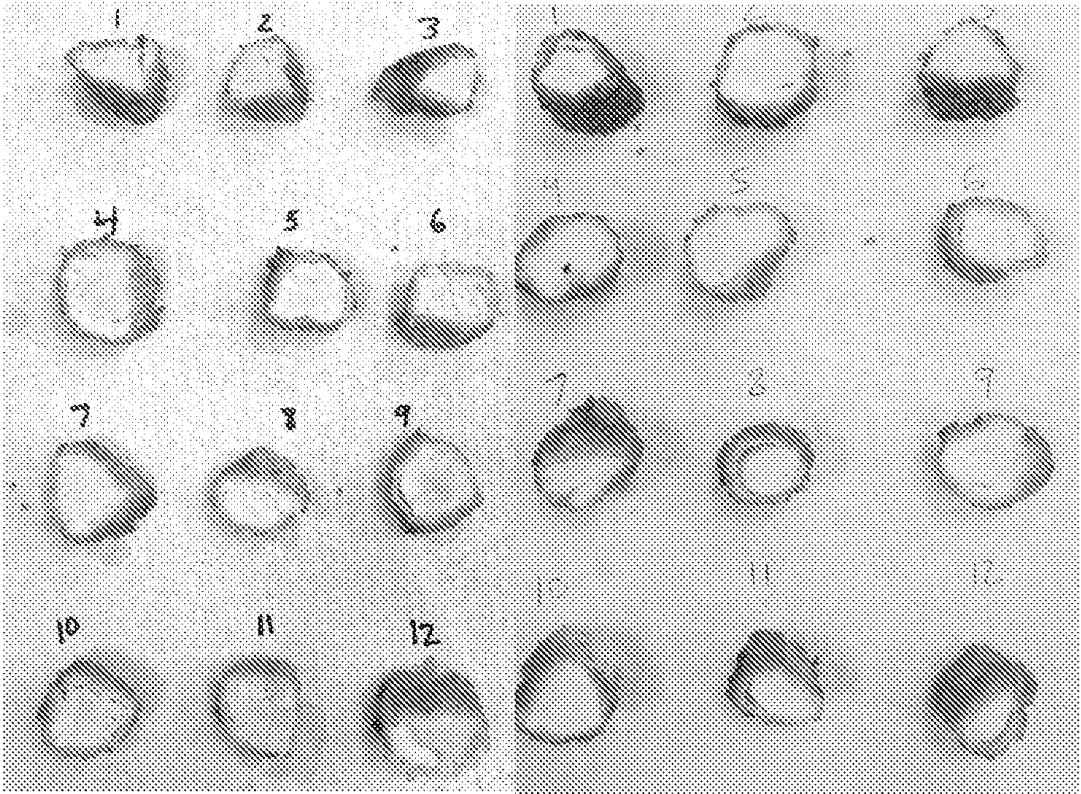
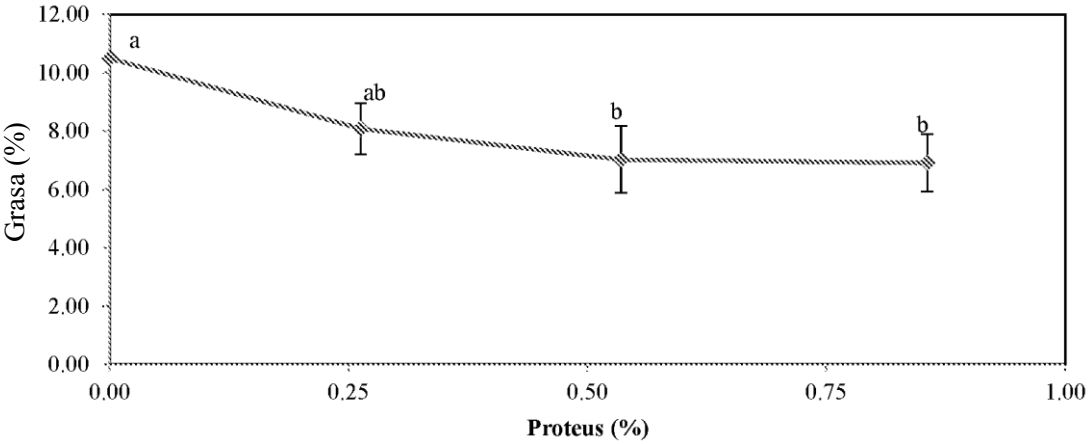


FIG. 26



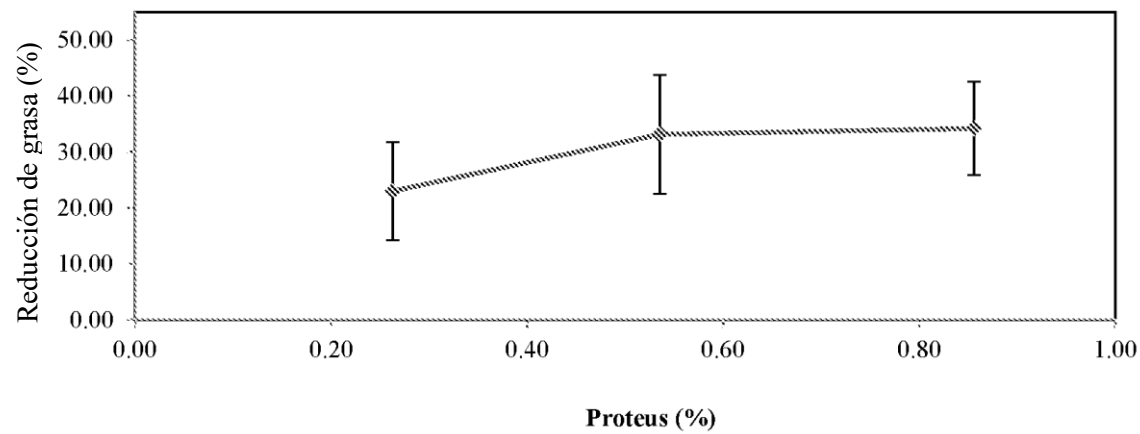


FIG. 28

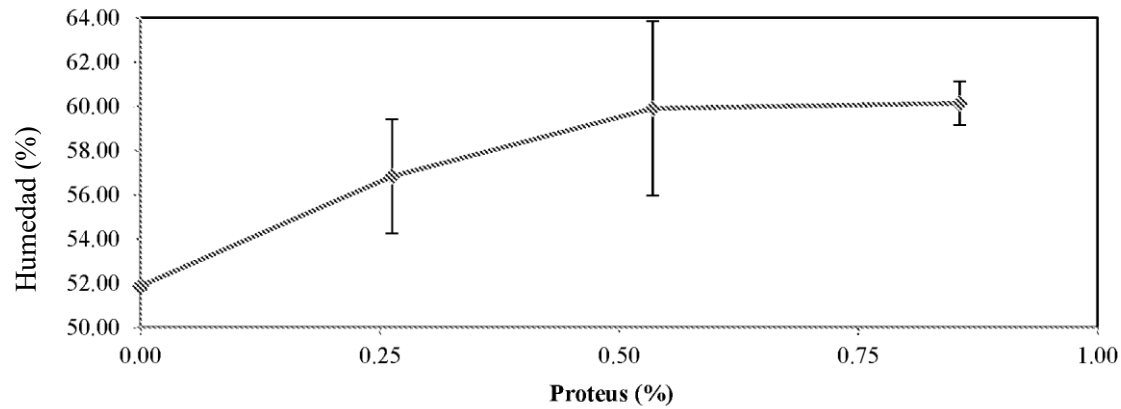


FIG. 29

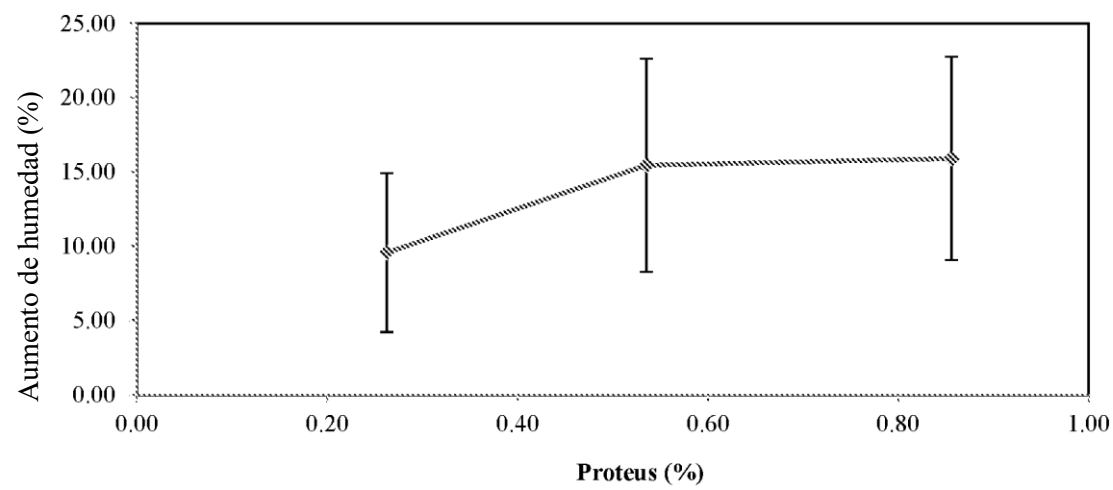


FIG. 30

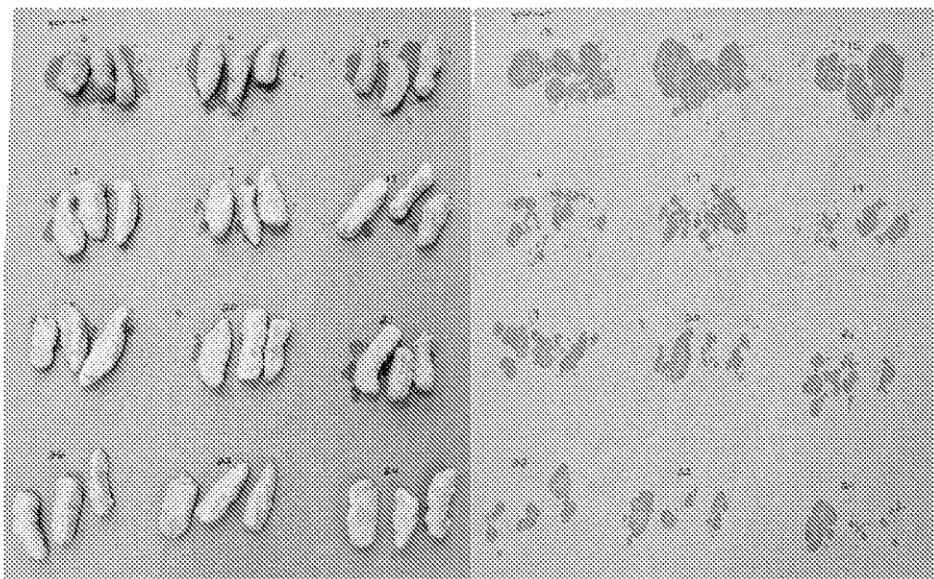


FIG. 31

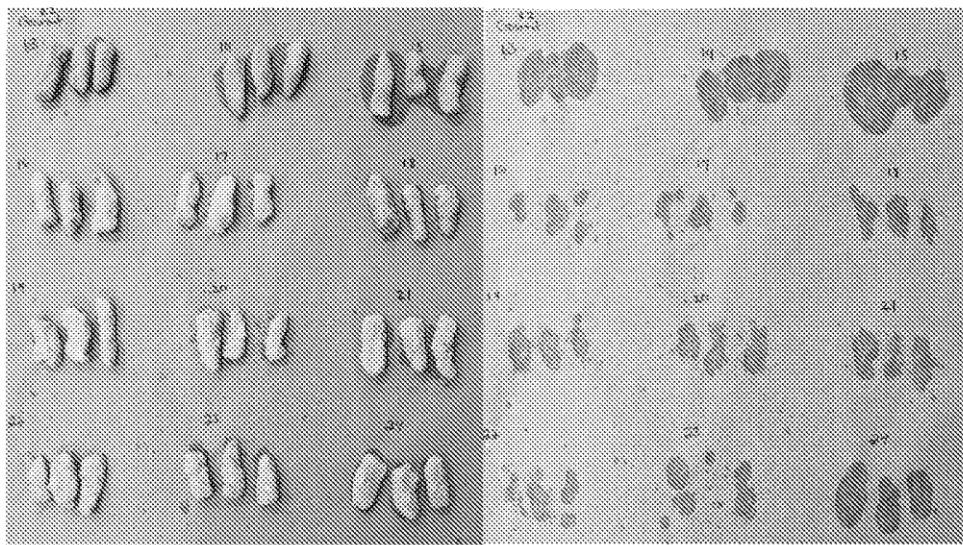


FIG. 32

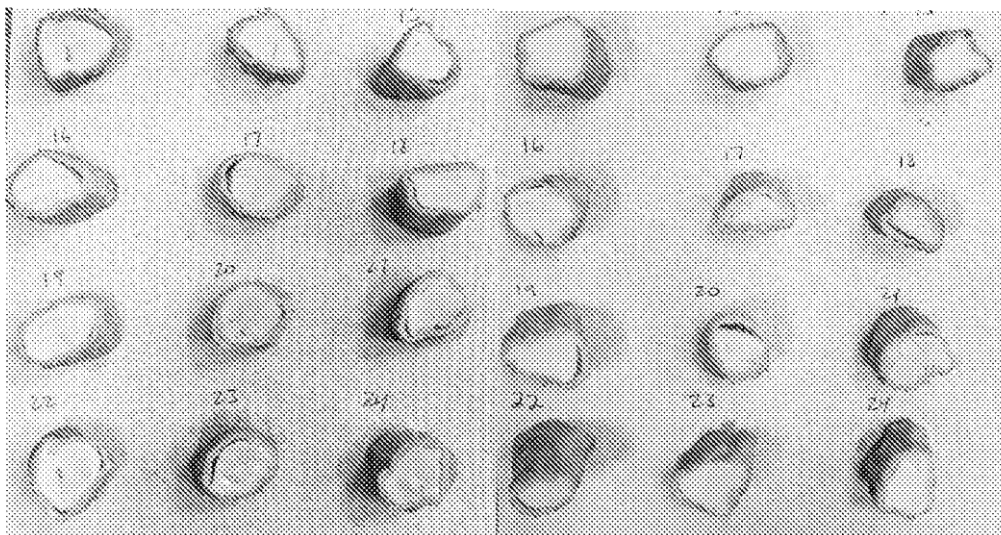


FIG. 33

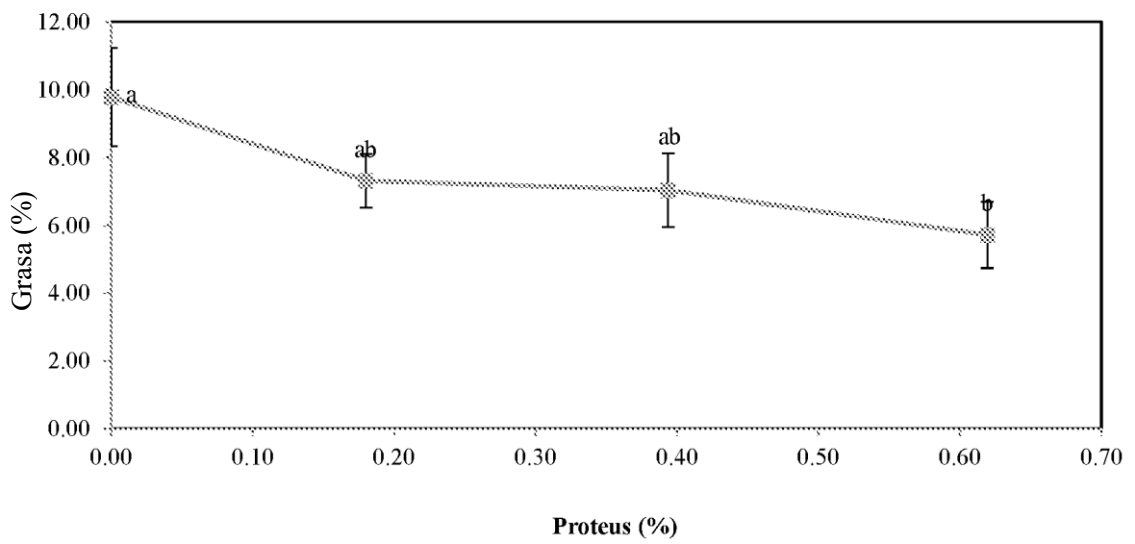


FIG. 34

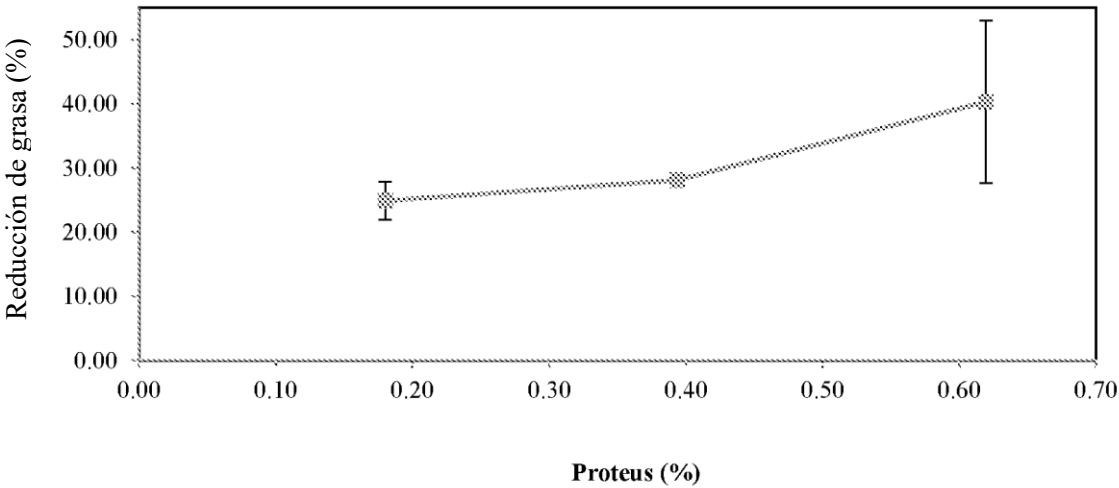


FIG. 35

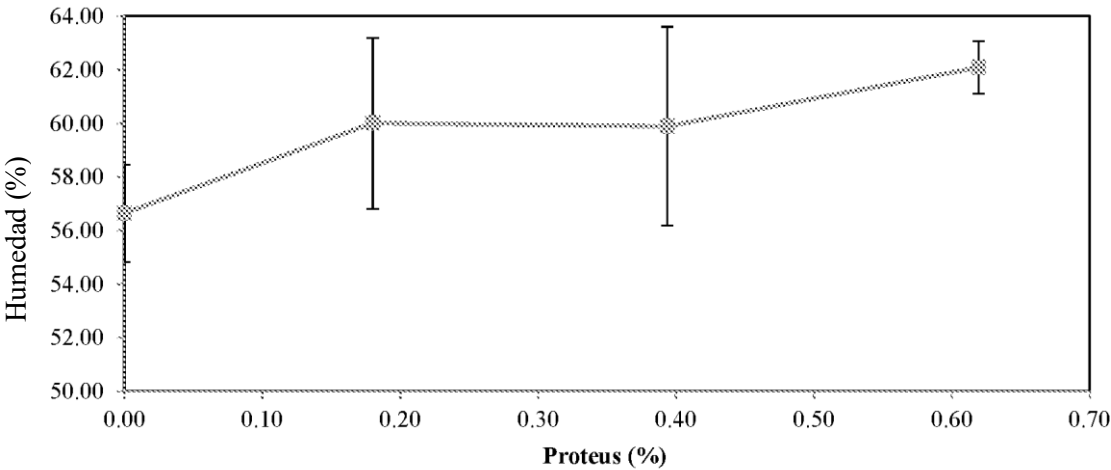


FIG. 36

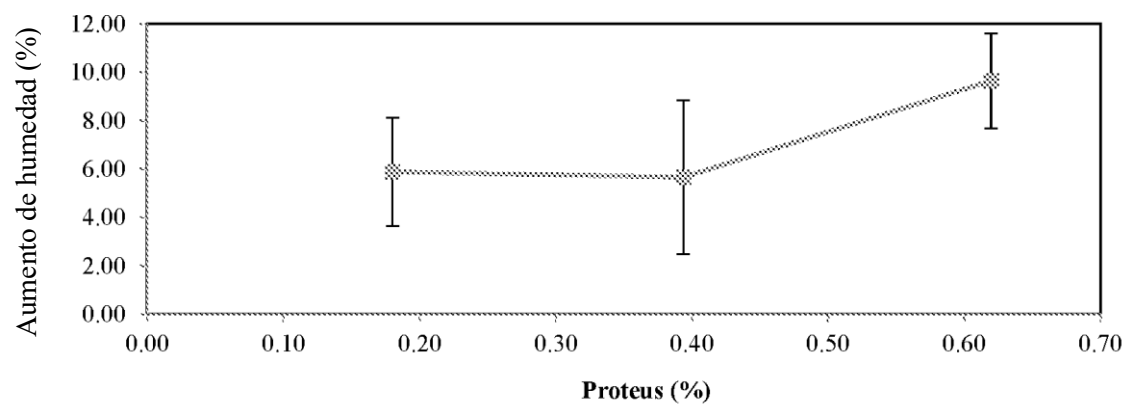


FIG. 37

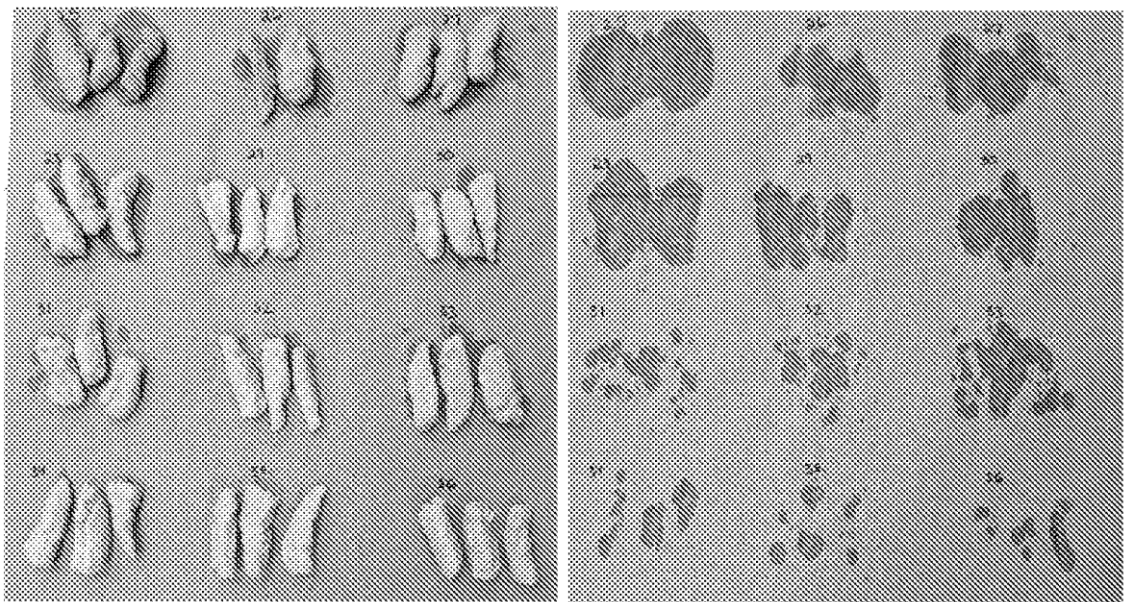


FIG. 38

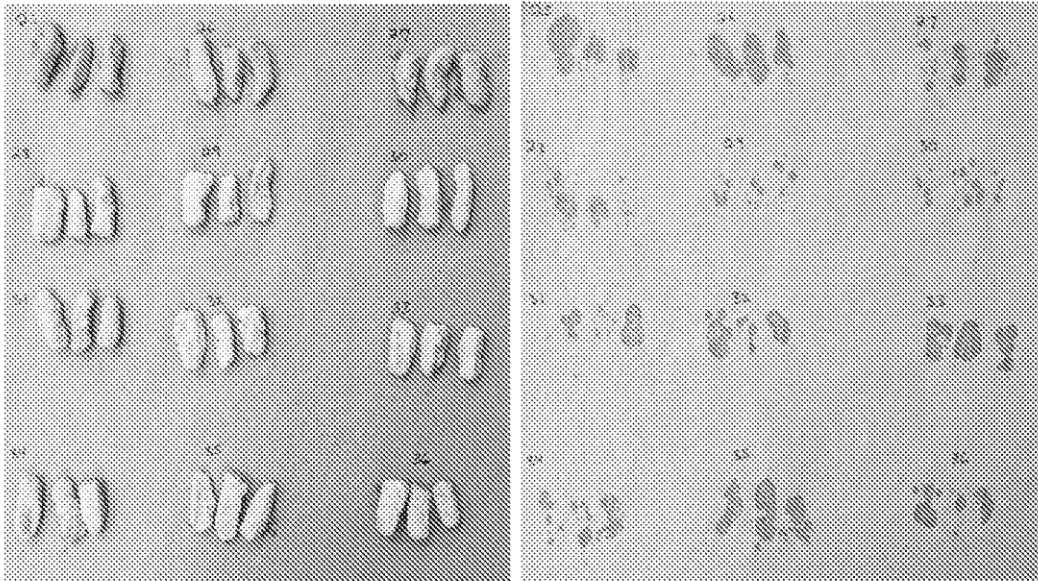


FIG. 39

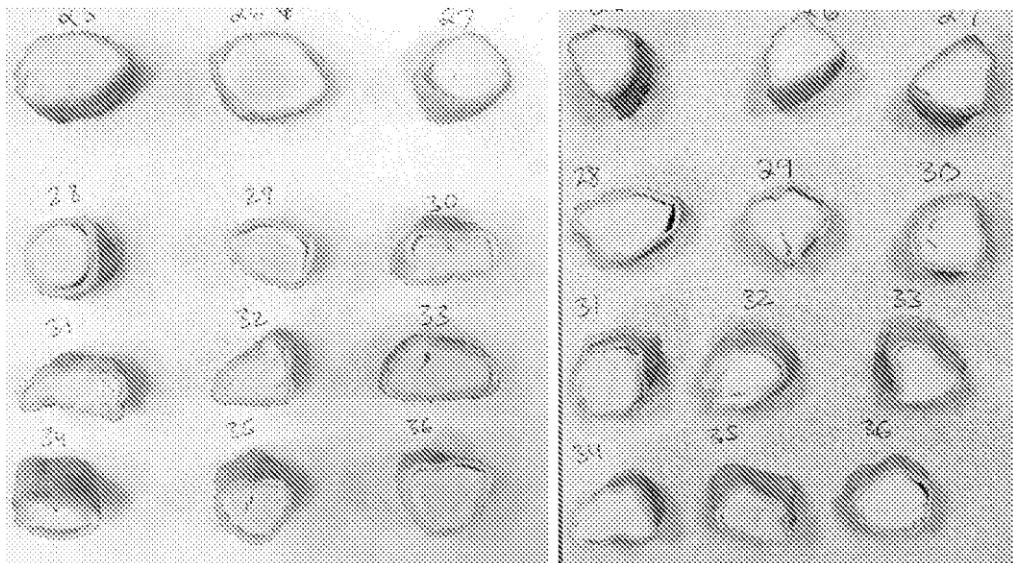


FIG. 40

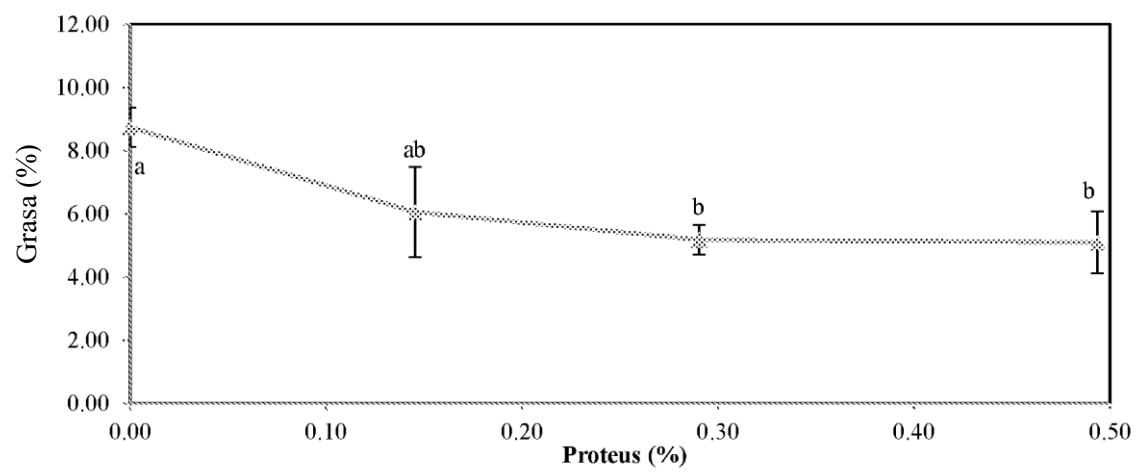


FIG. 41

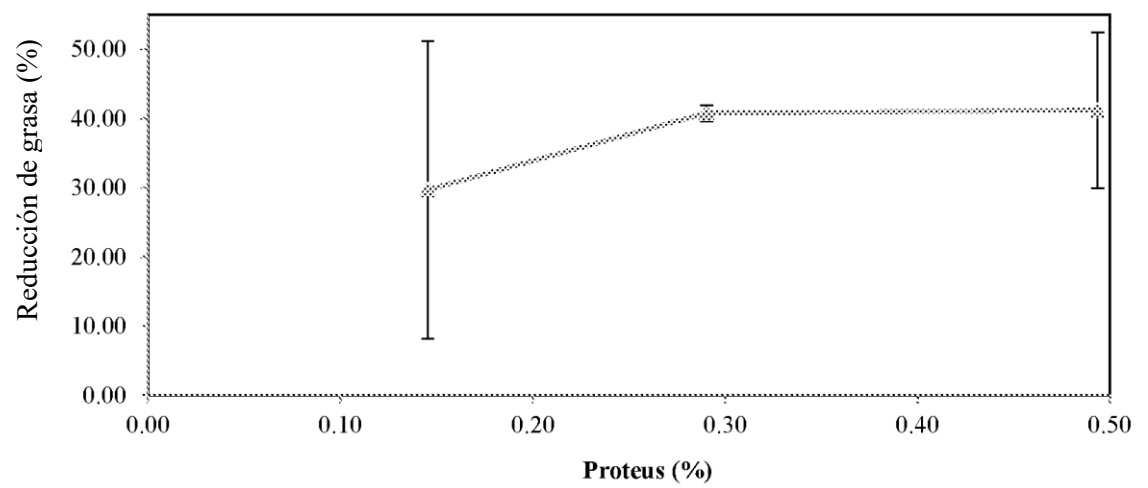


FIG. 42

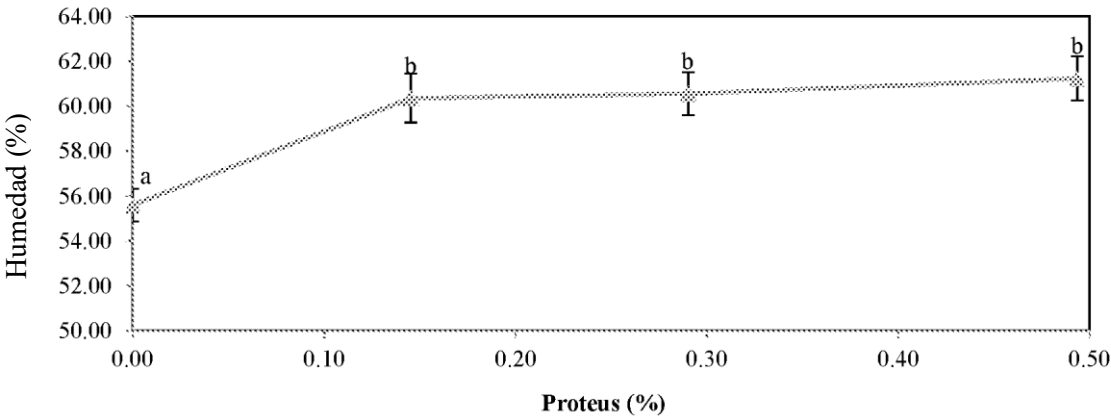


FIG. 43

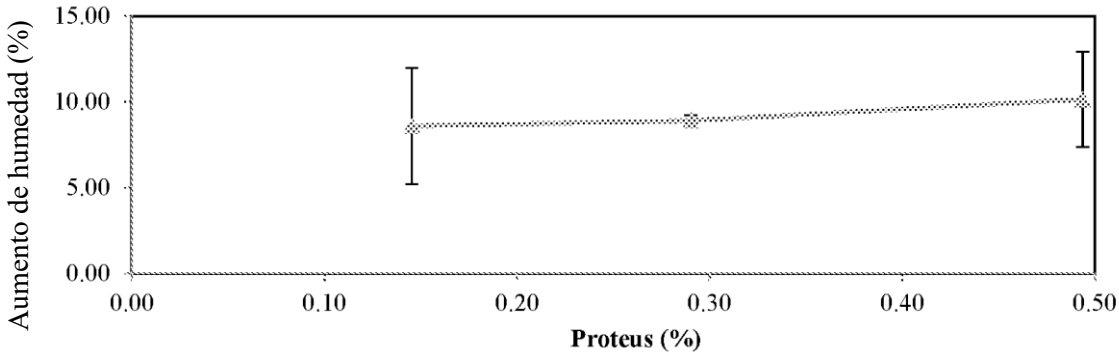


FIG. 44

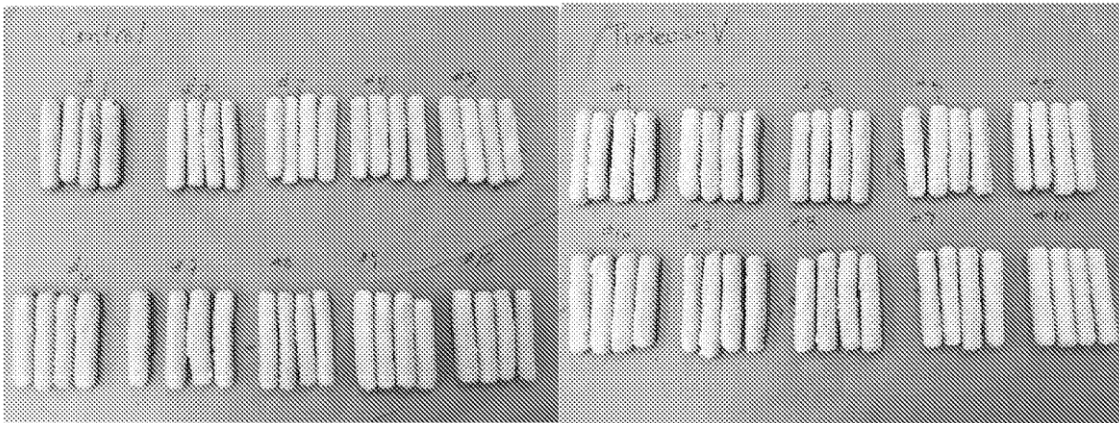


FIG. 45

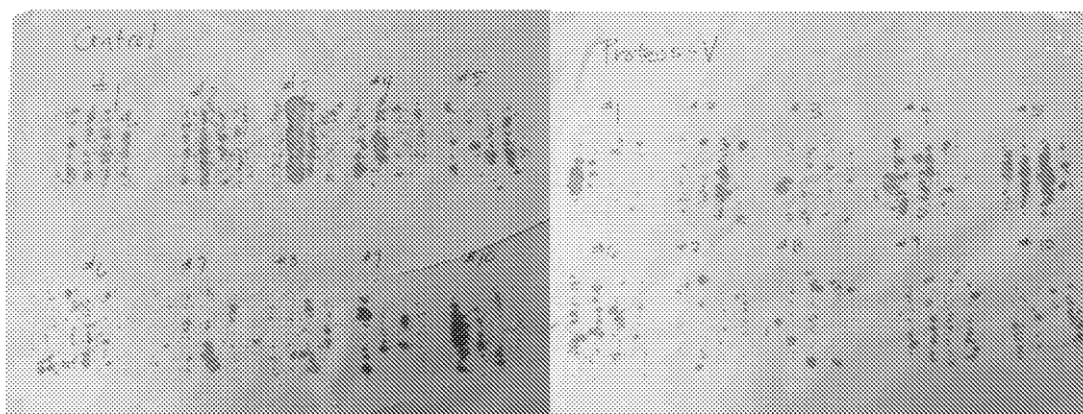


FIG. 46

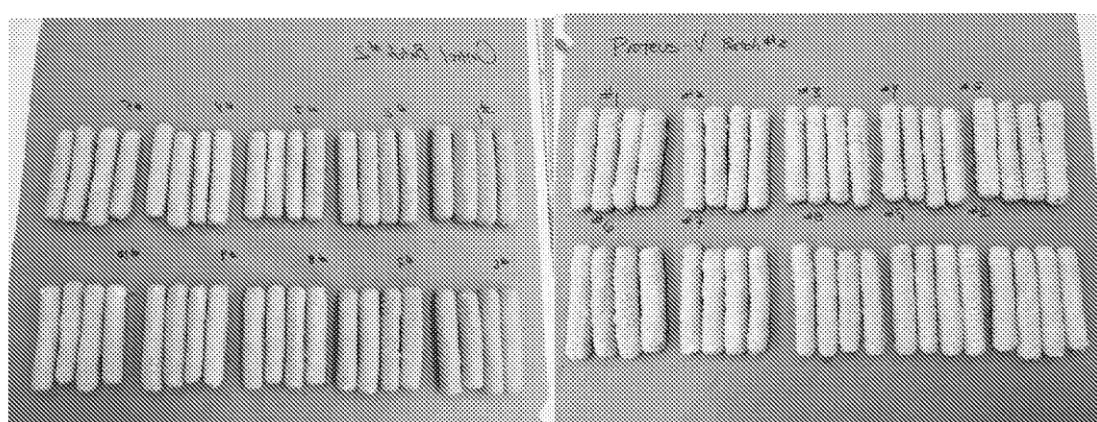


FIG. 47

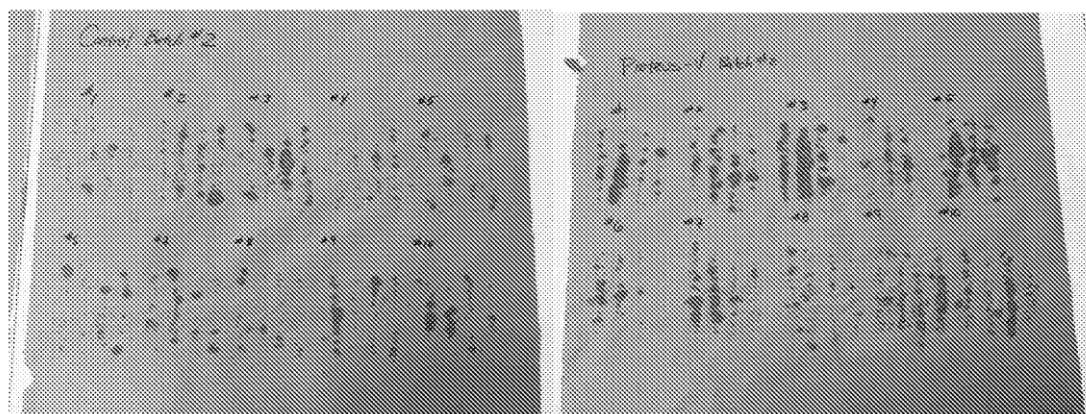


FIG. 48

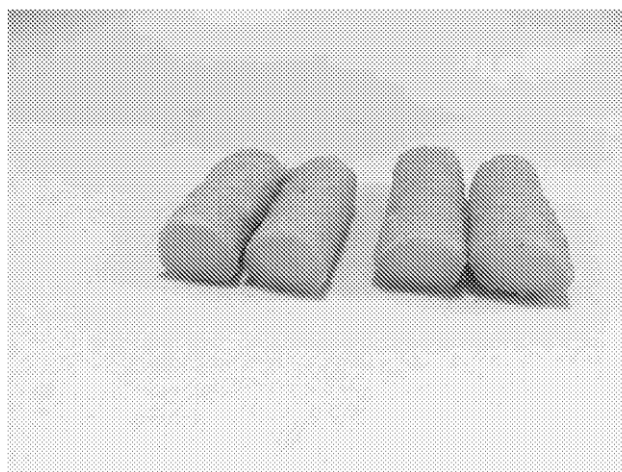


FIG. 49

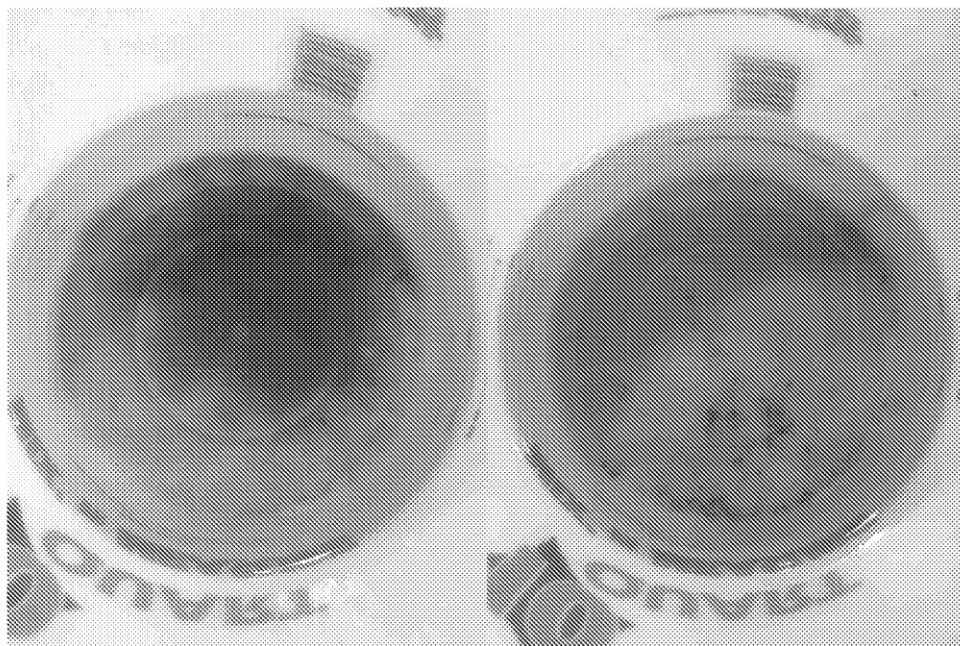


FIG. 50

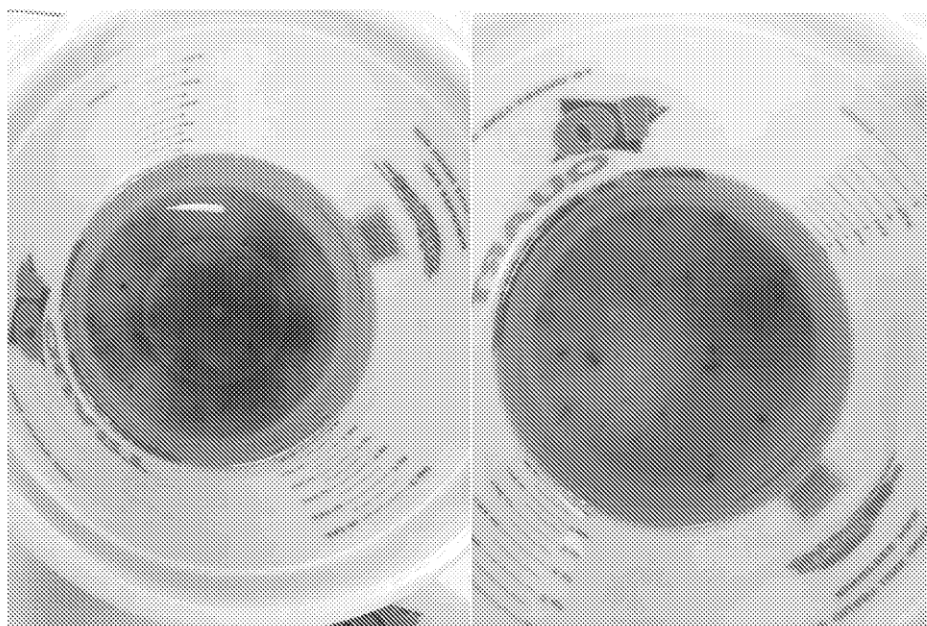


FIG. 51

110C Muestra	Peso de la muestra (g)	Tiempo de OSI (horas) Rep 1	Tiempo de OSI (horas) Rep 2	Tiempo promedio de OSI (horas)	Desviación Estándar	Error Estándar	2X Error Estándar
Lote de control n.º 1	5	7.35	7.85	7.60	0.3536	0.2500	0.5
Proteus®-V Lote n.º 1	5	8.1	8.2	8.15	0.0707	0.0500	0.1
Lote de control n.º 2	5	6.15	5.95	6.05	0.1414	0.1000	0.2
Proteus®-V Lote n.º 2	5	6.6	7.3	6.95	0.4950	0.3500	0.7

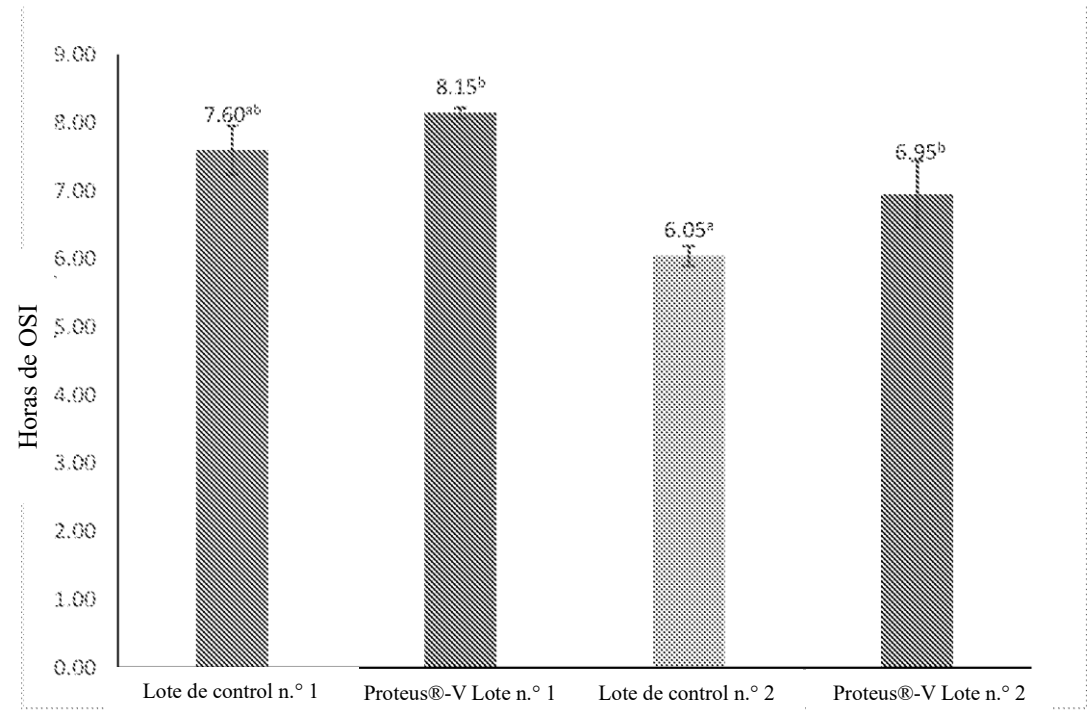


FIG. 52